


# KTO Tibial Intramedullary Nail System

CE 0197 ISO 13485 FDA



KANGLI ORTHOPAEDICS  
INSTRUMENT

## KTO Tibial Intramedullary Nail System

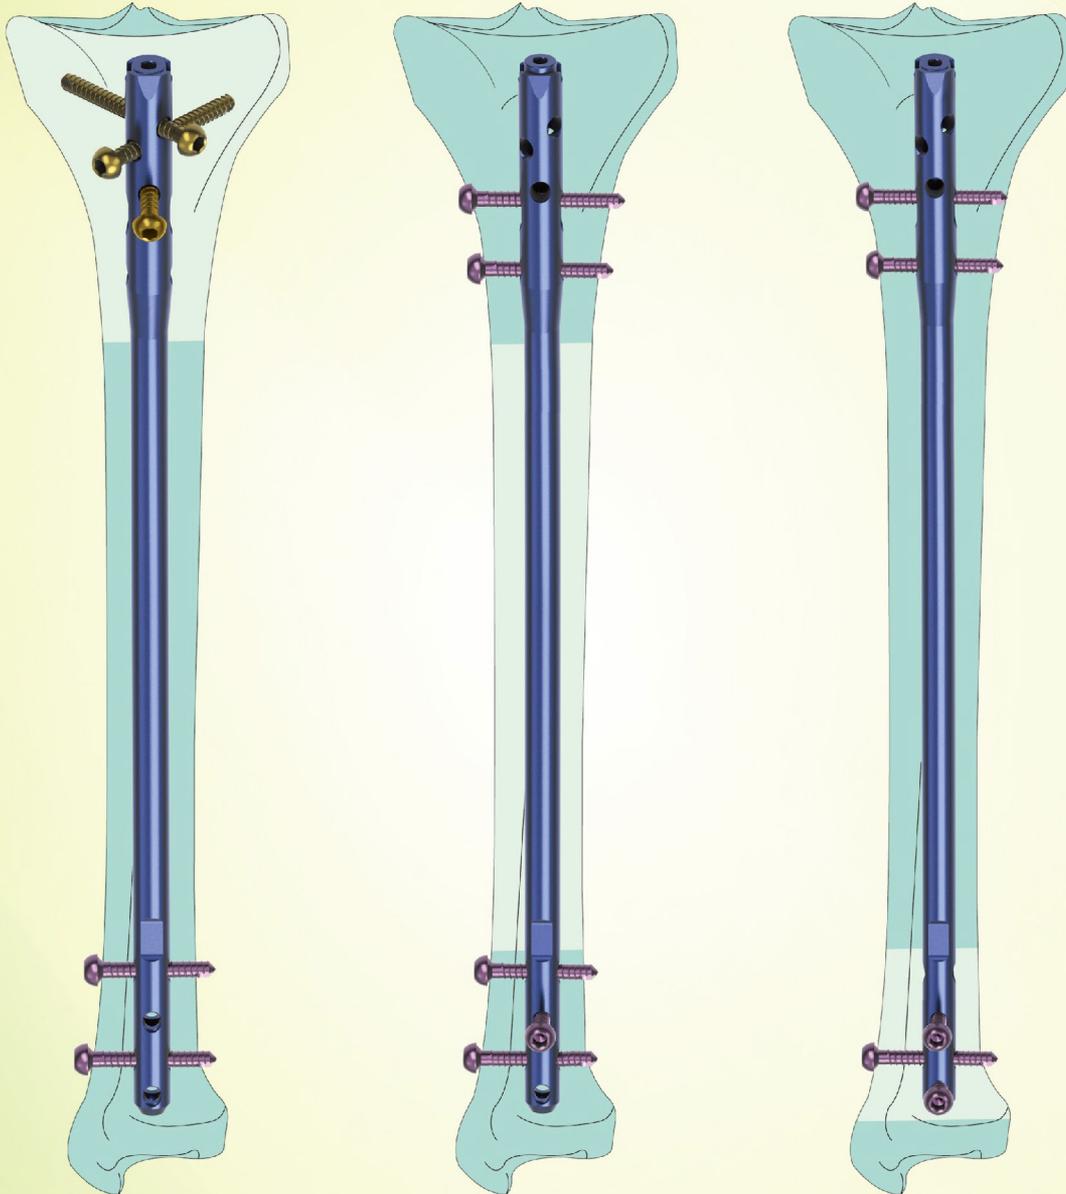

Fracture

## KTO Tibial Intramedullary Nail System

**KTO<sup>®</sup> Tibial Intramedullary Nail(Cannulated)**  
T8684、T8690、T8610



Product Name	Material	Diameter	Length	Product No.
KTO <sup>®</sup> Tibial Intramedullary Nail (Cannulated)	Titanium Alloy	Φ 8.4	255、270、285、300、315、330、345、360、375	T8684255- T8684375
		Φ 9.0	255、270、285、300、315、330、345、360、375	T8690255- T8690375
		Φ 10	255、270、285、300、315、330、345、360、375	T8610255- T8610375

**Φ4.5 Full Threaded Locking Screw**  
T852



Product Name	Material	Diameter	Length	Product No.
Full Threaded Locking Screw	Titanium Alloy	Φ 4.5	30	T8524030
			32	T8524032
			35	T8524035
			38	T8524038
			40、45、50、55、60、65、70、75、80	T8524040- T8524080

**Φ5.0 Full Threaded Locking Screw**  
T851



Product Name	Material	Diameter	Length	Product No.
Full Threaded Locking Screw	Titanium Alloy	Φ 5.0	40、45、50、55、60、65、70、75、80	T8515040- T8515080

**Normal End Cap**  
T8600001



Product Name	Material	Specification	Product No.
Normal End Cap	Titanium Alloy	0	T8600001

**Locking End Cap**  
T8600002



Product Name	Material	Specification	Product No.
Locking End Cap	Titanium Alloy	0	T8600002

### Supporting Instruments

